

Received: July 26, 2022  
Accepted: October 2, 2022

ISSN 1857–9027  
e-ISSN 1857–9949  
UDC:  
DOI:

*Original scientific paper*

## NANOMATERIALS IN VOLTAMMETRIC BIOSENSORS-RECENT ACHIEVEMENTS

**Rubin Gulaboski**

Faculty of Medical Sciences, Goce Delčev University, Štip, Republic of Macedonia

e-mail: rubin.gulaboski@ugd.edu.mk

While we inhabit a macro-world, it is evident that our future will depend greatly on the tiniest of things. This is due to the fact that a majority of 21st-century sciences will be centered around materials with nanometer dimensions. Currently, we observe the significance of nanomaterials in facilitating the targeted delivery of active substances within the body. In the past two years, this has played a crucial role in combating the COVID-19 pandemic, with the assistance of vaccines containing graphene oxide nanoparticles that serve as carriers and enhancers for vaccine compounds. Furthermore, challenges related to drug delivery, such as poor water solubility and limited bioavailability, have already been overcome through the utilization of metal-based and carbon-based nanomaterials. Nanomedicine is poised to revolutionize the landscape of therapeutics and diagnostics. This brief review focuses on notable achievements in designing specific voltammetric biosensors using metallic nanoparticles and graphene-based nanomaterials. Metallic nanoparticles, particularly those based on silver and gold, along with graphene derivatives such as nanotubes, quantum dots, nanodiamonds, and fullerenes, exhibit remarkable physical and chemical properties. These include improved thermal stability, enhanced conductivity, and the ability to modify their surface area with various organic substrates. Notably, voltammetric sensors based on graphene nanostructures demonstrate high biocompatibility and superior selectivity in detecting important biological systems through voltammetry. The aim of this concise review is to highlight recent electrochemical advancements in nanosystems and present significant achievements of metallic nanoparticles and graphene-based nanomaterials as voltammetric biosensors.

**Key words:** metallic nanoparticles; graphene; carbon nanotubes; electrochemical biosensors, voltammetry

### INTRODUCTION

Voltammetry is arguably the most valuable electrochemical technique for gaining insights into various aspects of electrode transformations in physiological and chemical systems, ranging from small ions to large lipophilic proteins and enzymes [1–3]. As voltammetry revolves around measuring the energy of electrons exchanged between specific analytes and an electronic conductor (the working electrode), it becomes evident that the nature of the working electrode plays a crucial role in this electrochemical technique. A limited selection of working electrodes, primarily composed of noble metals, mercury, or carbon materials, have been reported as suitable materials for the majority of voltammetric studies [1, 4–6]. The effective utilization of volt-

ammetry for probing specific ions, drugs, or physiologically active systems at micromolar or lower concentrations often necessitates the modification of working electrode surfaces with materials possessing superior conductive and chemical properties compared to unmodified electrodes [7]. Over the past 20 years, extensive exploration has been carried out on various nanomaterials to enhance the surfaces of electronic conductors used in voltammetric experiments [8]. Among these, nanoparticles based on metals (such as Au, Ag, Pt), metal oxides (primarily Fe<sub>2</sub>O<sub>3</sub>, Al<sub>2</sub>O<sub>3</sub>, CuO, CoO, MoO<sub>3</sub>, Bi<sub>2</sub>O<sub>3</sub>), and particularly those derived from different carbon materials (multiwalled and single-walled carbon nanotubes) have been widely employed in voltammetric systems. Their usage has significantly contributed to the successful application of voltammetry in the de-


sign of numerous voltammetric sensors for detecting important chemical and physiological compounds [1, 5]. This brief overview highlights some of the key achievements of nanomaterials in the development of voltammetric sensors in recent years.

## RESULTS AND DISCUSSION


The concept of "nanotechnology," initially developed by Richard Feynman [9] (Nobel Prize laureate in 1965), has brought about revolutionary advancements in the fields of nanomedicine, pharmacy, chemistry, physics, high-tech industry, food industry, and numerous other related fields [8, 10–12]. Nowadays, nanomaterials have become ubiquitous in every aspect of our lives. Over the past 20 years, nanotechnology has made significant impacts in areas such as drug delivery, cancer therapy, drug synthesis, cellular phones and computer technology, development of new materials, high-precision electronics, and environmental analysis. Although nanoparticles (NPs) encompass a wide range of materials, they are commonly defined as "three-dimensional materials with at least one dimension in their structure measuring less than 100 nm" [11]. Numerous excellent books have been published in the last 15 years, covering important topics related to the synthesis, properties, functions, characterization, and applications of various NPs. Interested readers are advised to refer to some of these publications [13–20]. In general, the remarkable characteristics of nearly all nanoparticles (NPs) that render them highly suitable for implementation in electrochemical systems are attributed to their exceptional catalytic properties, larger surface area-to-volume ratio achieved by reducing their size, improved electronic conductivity, enhanced durability, and com-

patibility with various substrates. Additionally, many NPs, particularly those based on graphene, serve as favorable platforms for attaching functional groups, which is an important feature manifested in their reactivity towards specific substrates. While numerous recent excellent reviews cover different properties, synthesis protocols, characterization, and application of nanoparticles in electrochemical experiments [21–26], this overview focuses on highlighting only a selection of the most significant properties and achievements of certain types of nanoparticles utilized in voltammetric biosensing. Figure 1 illustrates a scheme showcasing some of the key NPs employed in electrochemistry, while Figure 2 depicts a modified working electrode with gold nanoparticles, suitable for voltammetric experiments.

The initial mention of metal nanoparticles in electrochemistry dates back more than 30 years [11]. Metal nanoparticles are highly attractive for modifying various electrode surfaces due to their easy and cost-effective preparation, as well as their notable electrocatalytic properties [11, 14, 26]. When attached to the working electrode, these nanoparticles significantly increase its active surface area due to their small size. Furthermore, the use of metallic nanoparticles commonly enhances the material's electrical conductivity, leading to an increased rate of electron exchange between the studied analytes and the modified electrodes [4–8, 14]. Among the metallic nanoparticles investigated in voltammetric studies, silver and gold nanoparticles are the most well-known [14, 21]. This is primarily attributed to their relatively inexpensive and straightforward synthesis protocol, often involving chemical reduction from salt solutions using mild reductive substances such as citric acid [11, 14].

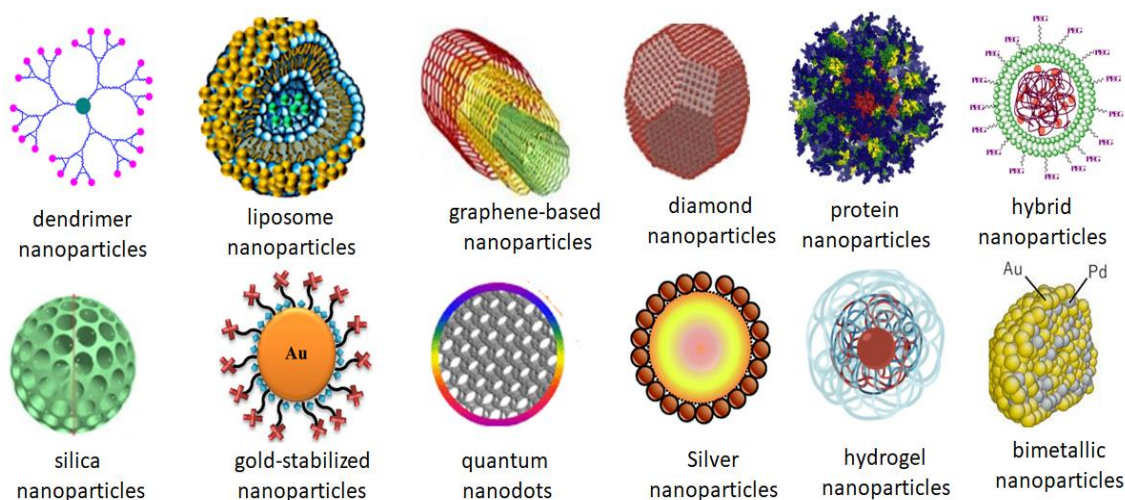

**Figure 1.** Schemes of some nanoforms mostly used in electrochemical experiments

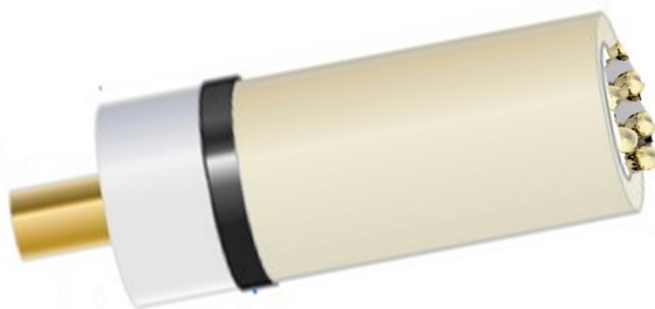

**Figure 2.** Schematic representation of a working electrode, with active electrode surface modified with gold nanoparticles

Another advantage of utilizing silver and gold nanoparticles is their potential for stabilization and modification with various ligands and functional groups on their surfaces [26]. In the case of modifying working electrodes with silver nanoparticles, electrodeposition under controlled potential is also feasible and easily achievable, as reported in [14-17]. When silver nanoparticles are combined with graphene oxide, the reduction of silver nitrate from a water solution is commonly accomplished using hydrogen iodide as a reducing agent [27]. A chemical reduction protocol allows the production of silver nanoparticles with sizes ranging between 10 nm and 25 nm [28]. On the other hand, electrodeposition of silver nanoparticles typically results in larger particles with diameters ranging between 30 and 50 nm [27]. Unfortunately, aggregation of deposited silver nanoparticles into larger clusters often occurs and is difficult to avoid when using the electrodeposition method. The toxicity of silver nanoparticles is recognized as a significant drawback when applying these materials in experiments involving physiological systems. Gold nanoparticles are among the most extensively studied metallic nanomaterials for electrochemical detection of different analytes [29, 30]. The most common method for obtaining gold nanoparticles is through chemical reduction of chloroauric acid in water solutions using mild reducing agents such as sodium citrate, ascorbic acid, and sodium borohydride [11, 14]. An advantageous characteristic of gold nanoparticles is their ability to form covalent bonds with substrates containing thiol (-S-H) groups in their structure [14]. Numerous modification protocols involving "mercapto substrates" [31] have paved the way for the widespread use of thiol-modified gold nanoparticles in voltammetric sensing, particularly for the quantification of important biomolecules like DNA [32]. Other metallic and bimetallic nanoparticles derived from bismuth, platinum, copper, nickel, cobalt, titanium, palladium, mercury, and various other metals have

also been extensively employed in various voltammetric studies [13-15]. In addition to metallic nanoparticles, metal-oxides and metal-sulfides nanoparticles have been extensively explored for voltammetric purposes over the last 10 years. Detailed information regarding their synthesis protocols, properties, functions, and applications can be found in comprehensive reports such as [14, 33-36]. Table 1 summarizes some of the most significant applications of metallic, metal-oxides, and metal-sulfides nanoparticles in voltammetric sensing of chemical and physiological systems, as published in recent years.

A significant turning point in experimental voltammetry occurred approximately 20 years ago, coinciding with the isolation of freestanding graphene [51]. The integration of this two-dimensional carbon material in electrochemical experiments marked the beginning of a new era in the development of voltammetric sensors for probing important chemical and physiological systems [52]. Due to its ability to be easily wrapped and rolled, graphene became a fundamental building block in the design of various carbon-based nanomaterials, including carbon single-walled and multi-walled nanotubes, fullerene, nanoplatelets, and other nanoforms [53]. Over the past 15 years, graphene has consistently demonstrated superior performance compared to existing electrode materials when used as a modifier for electrochemical sensors. Analysis of voltammetric sensors published since 2012 indicates that more than 30% of the works report the exploration of graphene-based nanomaterials (primarily single-walled and multi-walled carbon nanotubes) for the modification of electrode surfaces [51].

The extensive exploration of 3D graphene-based nanoforms in voltammetric biosensors can be attributed to their remarkable features, including their exceptional electrical conductivity, high chemical stability, and their ability to serve as platforms

**Table 1.** Data about voltametric detection of different substrates with metal-based nanoparticles

Type of nanoparticles	Voltammetric Technique/ Working Electrode	Analyte	Detection limit of the analyte	Reference
Au-nanoparticles stabilized with dithiothreitol and dodecanethiol	DPV/Au electrode	epinephrine	0.06 $\mu\text{mol/L}$	[37]
various Au-nanoparticles	DPV and SWV/GCE/Au electrode	various polyphenols	in sub-micromolar range	[38]
Au-nanoparticles	CV/GCE	glutathione	0.7 pmol/L	[38]
Au-nanoparticles stabilized with various substrates	DPV, SWV and CV /GCE/Au electrode	DNA	sub-micromolar concentrations	[32]
various metallic nanoparticles	DPV, SWV and CV/GCE/Au electrode	hazardous polyphenols in water	sub-micromolar concentrations	[40]
Ag-nanoparticles/multi-walled nanotubes	DPV/GC electrode	glucose	0.01 mmol/L	[41]
Pt-Ag nanoflowers	DPV/GC electrode	hydrogen peroxide, glucose	0.02 mmol/L	[42]
various metallic and bimetallic nanoparticles	DPV, SWV and CV /GCE/Au/Pt electrode	$\text{Sb}^{2+}$ , $\text{As}^{5+}$ , $\text{Cd}^{2+}$ , $\text{Cr}^{6+}$ , $\text{Cu}^{2+}$ , $\text{Pb}^{2+}$ , $\text{Hg}^{2+}$ , $\text{Ni}^{2+}$	mainly in sub-micromolar concentrations	[33]
Au-nanoparticles	DPV/GCE	glucose and hydrogen peroxide	for glucose 0.39 $\mu\text{mol/L}$ for hydrogen peroxide 0.136 $\mu\text{mol/L}$	[43]
CuO nanowires	CV/copper foam	glucose	lower mmol/L range	[44]
Au-Pd/MoS <sub>2</sub>	CV/GCE	glucose and hydrogen peroxide	for glucose 0.16 $\mu\text{mol/L}$ for hydrogen peroxide 0.40 mmol/L	[45]
Pd-nanoparticles on Co-wrapped carbon nanotubes	CV/GCE	hydrazine	0.07 $\mu\text{mol/L}$	[46]
Au-nanoparticles stabilized with mercaptoundecanoic acid	CV/SWV/GCE	vitamin E	0.25 $\mu\text{mol/L}$	[47]
Au-nanoparticles stabilized with mercaptoundecanoic acid	CV and SWV/GCE	DNA	7.5 $\mu\text{mol/L}$	[47]
Ag-nanoparticles at water-nitrobenzene interface	SWV and CV/GCE and PIGE	inorganic anions transferred across liquid-liquid interface	0.1 mmol/L	[48]
Ag/MoS <sub>2</sub> hybrid nanoparticles	CV/ITO	dopamine	lower mmol/L concentration range	[49]
Fe <sub>3</sub> O <sub>4</sub> nanoparticles-polyvinyl chloride	CV/Sn electrode	glucose	8 $\mu\text{mol/L}$	[50]


\* CV-cyclic voltammetry; SWV-square-wave voltammetry; DPV-differential pulse voltammetry;

\*\* GCE-glassy carbon electrode; PIGE-paraffin impregnated graphite electrode; ITO-indium tin oxide electrode

for attaching various substrates with specific functional groups onto their surfaces [54].

To harness the extraordinary features of carbon nanotubes (CNTs) for the development of voltammetric sensors, they typically undergo initial functionalization with biocompatible molecules [55]. This functionalization step yields a bio-modified nanointerface that serves as a crucial platform for designing specific voltammetric biosensors. Various organic or inorganic substrates are commonly employed for the functionalization of

CNTs, resulting in improved properties such as enhanced chemical compatibility and increased water solubility [53-55]. "Covalent functionalization" primarily involves small molecules that induce changes in the  $\pi$ -electronic framework of graphene [56]. On the other hand, "noncovalent functionalization" of these nanomaterials involves interactions between graphene's structure and aptamers, enzymes, polymers, and other organic systems (as illustrated in Figure 3), typically achieved through van der Waals interactions [56].

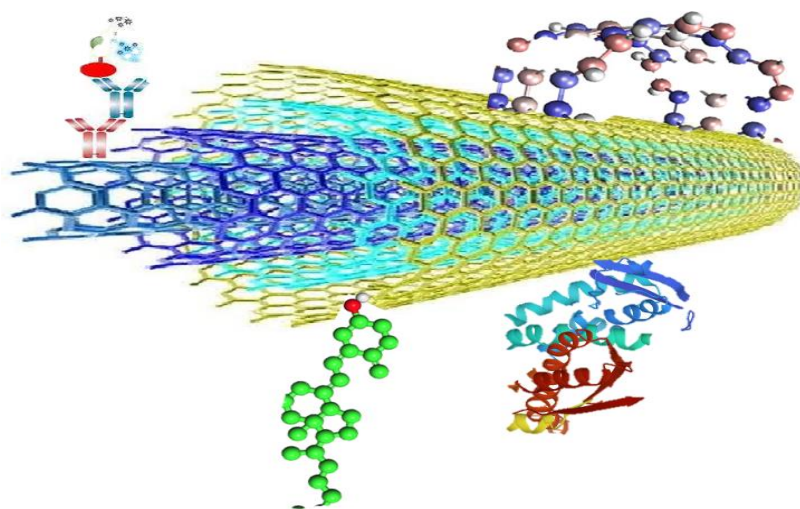

**Figure 3.** Scheme of a multiwalled carbon nanotubes that are functionalized with various organic molecules. The functionalization of carbon nanotubes with organic molecules is seen as a key step in achieving better selectivity of carbon nanomaterials.

Carbon nanoparticles, including graphene-made nanoparticles, have a propensity to induce changes in the electrical and chemical properties of non-modified electrodes. This often leads to significantly improved overall electrochemical performance of nano-modified electrodes for the detection of specific target molecules [56]. Over the past two decades, tens of thousands of papers have been published on electrochemical biosensors utilizing graphene-based nanoparticles in various forms, such as amperometric enzyme electrodes, voltammetric immunosensors, and nucleic acid voltammetric devices. In recent years, several comprehensive reviews have focused on graphene-based nanomaterials in the design of voltammetric biosensors suitable for quantifying diverse analytes, including DNA, dopamine, glucose, various hem-containing redox proteins, cytochromes, hormones, ascorbic acid, hydrogen peroxide, bilirubin, various pharmaceuticals, and other physiological systems. Interested readers are encouraged to refer to these works [52-61].

Enzyme-based electrochemical biosensors find extensive use in pharmacy, nanomedicine, food safety, and studies related to monitoring different substances relevant to environmental protection [53-56, 58].

Numerous voltammetric biosensors utilizing CNT-modified electrodes provide valuable insights into the activity of various redox enzymes [see reviews 58, 62, 63, and references therein]. Clinical biochemistry, being a major application area for biosensors, has witnessed a plethora of studies dedicated to the development of voltammetric biodevices for monitoring glucose, hemoglobin, urea, and other relevant physiological systems in whole blood [see reviews 58, 62-64, and references therein]. Additionally, over the past 10 years, there has been intensive exploration of graphene-based nanomaterials in designing reliable voltammetric biomarkers for medical diagnostics [65-67]. Table 2 provides information on some of the noteworthy recent achievements in the design of voltammetric biosensors using various graphene-based nanomaterials.

**Table 2.** Data about voltammetric detection of different substrates with graphene-based nanoparticles

Type of graphene-based nanoparticles	Voltammetric Technique/ Working Electrode	Analyte	Detection limit of the analyte	Reference
Multiwalled carbon nanotubes functionalized with cysteamine	CV/GCE	hemoglobin	0.03 $\mu\text{mol/L}$	[68]
Multiwalled carbon nanotubes immobilized on gelatin + glucose oxidase	CV/GCE	glucose	0.5 mmol/L	[69]
Multiwalled carbon nanotubes on poly(vinyl alcohol)+ alcohol dehydrogenase	CV/GCE	ethanol	0.16 $\mu\text{mol/L}$	[70]
multiwalled carbon nanotubes	CV/GCE	Cholesterol	0.5 $\mu\text{mol/L}$	[71]
multiwalled carbon nanotubes-metal oxide nanoparticles-7, 7, 8, 8-tetracyanoquinodimethane	CV/GCE	xanthine	0.2 $\mu\text{mol/L}$	[72]
composite of dendrimer-encapsulated Pt nanoparticles and carbon nanotubes	CV/GCE	Ascorbic acid, hydrogen peroxide	10 $\mu\text{mol/L}$ 50 $\mu\text{mol/L}$	[73]
multi-copper enzyme co-adsorbed at carbon nanotube	CV/GCE	Hydrogen peroxide	lower micromolar range	[74]
dehydrogenase modified quantum dots-carbon (ZnS-CdS) nanotubes	CV/GCE	glucose	10 $\mu\text{mol/L}$	[75]
Hybrid of silver multiwalled carbon nanotubes/manganese dioxide.	CV/GCE	carcino-embryonic antigen	10 $\mu\text{g/L}$	[76]
Multiwalled carbon nanotubes	CV/GCE	paracetamol ibuprofen	1 $\mu\text{mol/L}$ 1 $\mu\text{mol/L}$	[77]
carbon black nanoparticles	CV/GCE	hemoglobin	lower micromolar range	[78]
carbon black nanoparticles	CV/GCE	various hem-containing proteins	below 1 $\mu\text{mol/L}$	[79]
epoxy polymer and acetylene black nanoparticles	CV/GCE	Cytochrome P450	below 1 $\mu\text{mol/L}$	[80]

## OUTLOOKS FOR THE FUTURE

It is increasingly evident that the remarkable properties of metallic nanoparticles and the exceptional chemical performances of graphene-based nanomaterials will play a pivotal role in shaping scientific advancements in medicine, chemistry, pharmacy, physics, new materials design, and environmental analysis throughout the 21st century [58]. During the last three years of the Covid-19 pandemic, it has become evident that the efficient functioning of vaccines relies on the support of graphene-based nanomaterials [81]. Furthermore, the delivery of many important drugs in medicine is closely linked to the unique properties of carbon nanotubes

and fullerenes [82-86]. The remarkable electrochemical properties of graphene-based 3D nanomaterials have ushered in a new era of their widespread use in designing voltammetric biosensors for the detection of crucial biomolecules [58, 87]. As over 50% of novel works on voltammetric biosensors incorporate the use of nanomaterials, we anticipate a rapid breakthrough in the more extensive application of voltammetry in commercially designed devices [88].

To enhance the sensitivity and selectivity of nanomaterials, the development of novel nanomaterials with functionalized surfaces, incorporating multiple substrates within a single nano-platform, is anticipated. This advancement will enable the sim-

ultaneous and selective determination of different biomolecules in real-time [89]. From this perspective, it is highly likely that the remarkable chemistry of nanomaterials will soon lead to the emergence of novel fields in electrochemical research that will impact various aspects of our daily lives, particularly by improving biochemical, pharmaceutical, and medical research in numerous ways [81, 83, 90-92].

**Acknowledgment:** Rubin Gulaboski thanks the Alexander von Humboldt Foundation (Germany) for the support in 2021 during the research stay at Medical Faculty at Göttingen University, Germany (host, prof. Ivan Bogeski).

## REFERENCES

- [1] R. G. Compton, C. E. Banks, *Understanding Voltammetry*, 3<sup>rd</sup> Edition, World Scientific Publishing Europe Ltd, 2018.
- [2] V. Mirceski, S. Komorsky-Lovric, M. Lovric, *Square-wave Voltammetry-Theory and Application* (F. Scholz, ed.), Springer Verlag, Berlin, Heidelberg, 2007.
- [3] J. N. Butt, F. A. Armstrong, *Voltammetry of adsorbed redox enzymes*, in *Bioinorganic electrochemistry* (O. Hammerich, J. Ulstrup, eds), Springer, Netherlands, 2008.
- [4] A. J. Bard, L. R. Faulkner, *Electrochemical Methods: Fundamentals and Applications*, 2<sup>nd</sup> edition, John Wiley&Sons Inc., New York, 2001.
- [5] J. Wang, *Analytical Electrochemistry*, 3<sup>rd</sup> edition, John Wiley&Sons Inc., New York, 2006.
- [6] C. G. Zoski, *Handbook of Electrochemistry*, Elsevier, 2007.
- [7] R. Chillawar, K. K. Tadi, R. V. Motghare, Voltammetric techniques at chemically modified electrodes, *J. Anal. Chem.*, **70** (2015), pp. 399–418.
- [8] A. Chen, S. Chatterjee, Nanomaterials based electrochemical sensors for biomedical applications, *Chem. Soc. Rev.*, **42** (2013), pp. 5425–5438.
- [9] R. P. Feynman, There's plenty of room at the bottom, *Eng. Sci.*, **22** (1960), pp. 22–36.
- [10] N. Duran, P. D. Marcato, Nanobiotechnology perspectives. Role of nanotechnology in the food industry: A review. *Int. J. Food Sci. Technol.*, **48** (2013), pp. 1127–1134.
- [11] G. Cao, *Nanostructures and nanomaterials: Synthesis, properties and applications*, Singapore: Imperial College Press, 2004.
- [12] J. W. Schultze, A. Heidelberg, C. Rosenkranz, T. Schapers, G. Staikov, Principles of electrochemical nanotechnology and their application for materials and systems. *Electrochim. Acta*, **51** (2005), pp. 775–786.
- [13] *Fundamentals of nanoparticles*, (A. Barhoum, A. S. H. Makhlof, eds.), Elsevier, 2018.
- [14] *Inorganic Nanoparticles, Synthesis, applications, and perspectives*, (C. Altavilla, E. Ciliberto, eds.), CRC Press, 2010.
- [15] *Nanoparticles, workhorses of nanoscience*, (C. de Mello Donega, ed.), Springer, Berlin, Heidelberg, 2014.
- [16] *Nanoparticles: From theory to application*, (G. Schmid, ed.), Wiley, 2006.
- [17] *Nanoparticles in catalysis: Advances in synthesis and application*, (K. Philippot, A. Roucoux eds.), Wiley, 2021.
- [18] *Handbook of Nanophysics*, 1<sup>st</sup> edition, (K. D. Sattler, ed.), CRC Press, 2011.
- [19] *Nanoparticles for biomedical applications*, (E. J. Chung, L. Leon, C. Rinaldi, eds.), Elsevier, 2019.
- [20] C. S. Pundir, *Enzyme nanoparticles: Preparation, characterization, properties and applications (Micro and nano technologies)*, 1<sup>st</sup> edition, Elsevier, 2015.
- [21] S. E. F. Kleijn, S. C. S. Lai, M. T. M Koper, P. R. Unwin, Electrochemistry of nanoparticles, *Angew. Chem. Int. Ed.*, **53** (2014), pp. 3558–3586.
- [22] J. J. Jarju, M. C. Figueiredo, Y. V. Kolenko, *Chapter 8-Electrocatalysis using nanomaterials*, (A. J. Wain, E. J. F. Dickinson, eds.), *Frontiers of Nanoscience*, Elsevier, 18 (2021), pp. 343–420.
- [23] O. Lebedeva, D. Kultin, L. Kustov, Electrochemical synthesis of unique nanomaterials in ionic liquids, *Nanomaterials*, **11** (2021), pp. 3270. DOI: 10.3390/nano11123270
- [24] S-M. Lu, Y-Y. Peng, Y-L. Ying, Y-T. Long, Electrochemical sensing at a confined space, *Anal. Chem.*, **92** (2020), pp. 5621–5644.
- [25] Ib. Khan, K. Saeed, Id. Khan, Nanoparticles: Properties, applications and toxicities, *Arab. J. Chem.*, **12** (2019), pp. 908–931.
- [26] E. Katelhon, L. Chen, R. G. Compton, Nanoparticle Electrocatalysis: Unscrambling illusory inhibition and catalysis, *Appl. Mater. Today*, **15** (2019), pp. 139–144.
- [27] T. Han, J. Jin, C. Wang, Y. Sun, Y. Zhang, Y. Liu, Ag nanoparticles-modified 3D graphene foam for binder-free electrodes of electrochemical sensors, *Nanomaterials*, **7** (2017). DOI:10.3390/nano7020040
- [28] U. T. Khatoun, G. V. S. N. Rao, K. M. Mantravadi, Y. Oztekin, Strategies to synthesize various nanostructures of silver and their applications-A review, *RSC Adv.* **8** (2018), pp. 19739–19753.
- [29] S. Zeng, K.-T. Yong, I. Roy, X.-Q. Dinh, X. Yu, F. Luan, A Review on functionalized gold nanoparticles for biosensing applications, *Plasmonics*, **6** (2011), pp. 491–506.

- [30] S. Alex, A. Tiwari, Functionalized Gold Nanoparticles: Synthesis, Properties and Applications-A Review, *J. Nanosci. Nanotechnol.* **15** (2015), pp. 1869–1894.
- [31] S. J. Amina, B. Guo, A Review on the synthesis and functionalization of gold nanoparticles as a drug delivery vehicle, *Int. J. Nanomedicine*, **15** (2020), pp. 9823–9857.
- [32] M. T. Castaneda, S. Alegret, A. Merkoci, Electrochemical Sensing of DNA using gold nanoparticles, *Electroanalysis*, **19** (2007), pp. 743–753.
- [33] S. Sawan, R. Maalouf, A. Errachid, N. Jaffrezic-Renault, Metal and Metal Oxide Nanoparticles in the Voltammetric Detection of Heavy Metals: A Review, *TrAC-Trend. Anal. Chem.*, **131** (2020), 116014. <https://doi.org/10.1016/j.trac.2020.116014>
- [34] A. S. Agnihotri, A. Varghese, M. Nidhin, Transition metal oxides in electrochemical and bio sensing: A state of art, *App. Surf. Sci. Adv.*, **4** (2021), 100072. <https://doi.org/10.1016/j.apsadv.2021.100072>
- [35] E. Fazio, S. Spadaro, C. Corsaro, G. Neri, S. G. Leonardi, F. Neri, N. Lavanya, C. Sekar, N. Donato, G. Neri, Metal-oxide based nanomaterials: Synthesis, characterization and their applications in electrical and electrochemical sensors, *Sensors*, **21** (2021), 2494. <https://doi.org/10.3390/s21072494>
- [36] A. Balakrishnan, J. D. Groeneveld, S. Pokhrel, L. Madler, Metal sulfide nanoparticles: Precursor chemistry, *Eur. J. Chem.*, **27** (2021), pp. 6390–6406.
- [37] L. Wang, J. Bai, P. Huang, H. Wang, L. Zhang, Y. Zhao, Self-assembly of gold nanoparticles for the voltammetric sensing of epinephrine, *Electrochem. Commun.*, **8** (2006), pp. 1035–1040.
- [38] R. Petrucci, M. Bortolami, P. Di Matteo, A. Curulli, Gold nanomaterials-based electrochemical sensors and biosensors for phenolic antioxidants detection: Recent advances, *Nanomaterials* **12** (2022), 959 DOI: 10.3390/nano12060959
- [39] D. O. Pervezentseva, A. V. Korshunov, E. V. Gorchakov, V. I. Birmatov, I. E. Phedorov, Au-nanoparticles based sensors for voltammetric determination of glutathione, *Curr. Anal. Chem.*, **13** (2017), pp. 225–230.
- [40] B. R. Patel, M. Noroozifar, K. Kerman, Nanocomposite-based sensors for voltammetric detection of hazardous phenolic pollutants in water, *J. Electrochem. Soc.*, **167** (2020), 037568
- [41] L. Chen, H. Xie, J. Li, Electrochemical glucose biosensor based on silver nanoparticles/multiwalled carbon nanotubes modified electrode. *J. Solid State Electrochem.*, **16** (2012), pp. 3323–3329.
- [42] Z. Huang, A. Zhang, Q. Zhang, S. Pan, D. Cui, Electrochemical biosensor based on Dewdrop-like Platinum nanoparticles-decorated silver nanoflowers nanocomposites for H<sub>2</sub>O<sub>2</sub> and glucose detection, *J. Electrochem. Soc.*, **166** (2019) pp. B1138–B1145.
- [43] Z. Lu, L. Wu, J. Zhang, W. Dai, G. Mo, J. Ye, Bifunctional and highly sensitive electrochemical non-enzymatic glucose and hydrogen peroxide biosensor based on NiCo<sub>2</sub>O<sub>4</sub> nanoflowers decorated 3D nitrogen doped holey graphene hydrogel, *Mater. Sci. Eng. C*, **102** (2019), pp. 708–717.
- [44] Z. Li, Y. Chen, Y. Xin, Z. Zhang, Sensitive electrochemical nonenzymatic glucose sensing based on anodized CuO nanowires on three-dimensional porous copper foam, *Sci. Rep.*, **5** (2015) 1–8. <https://doi.org/10.1038/srep16115>.
- [45] X. Li, X. Du, Molybdenum disulfide nanosheets supported Au-Pd bimetallic nanoparticles for non-enzymatic electrochemical sensing of hydrogen peroxide and glucose, *Sensors Actuators B: Chem.*, **239** (2017), pp. 536–543.
- [46] Y. Zhang, B. Huang, J. Ye, J. Ye, A sensitive and selective amperometric hydrazine sensor based on palladium nanoparticles loaded on cobalt-wrapped nitrogen-doped carbon nanotubes, *J. Electroanal. Chem.*, **801** (2017), pp. 215–223.
- [47] R. Gulaboski, M. Chirea, C. M. Pereira, M. N. D. S. Cordeiro, R. B. Costa, A. F. Silva, Probing of the voltammetric features of graphite electrodes modified with mercaptoundecanoic acid stabilized gold nanoparticles, *J. Phys. Chem. C*, **112** (2008), pp. 2428–2435
- [48] V. Mirčeski, R. Gulaboski, Simple electrochemical method for deposition and voltammetric inspection of silver particles at the liquid-liquid interface of a thin-film electrode, *J. Phys. Chem. B*, **110** (2006), pp. 2812–2820.
- [49] J. W. Shin, J. Yoon, M. Shin, J. W. Choi, Electrochemical dopamine biosensor composed of silver encapsulated MoS<sub>2</sub> hybrid nanoparticle, *Biotechnol. Bioprocess. Eng.*, **24** (2019), pp. 135–144.
- [50] N. Sanaeifar, M. Rabiee, M. Abdollahi, M. Tahriri, D. Vashae, L. A. Tayebi, novel electrochemical biosensor based on Fe<sub>3</sub>O<sub>4</sub> nanoparticles-polyvinyl alcohol composite for sensitive detection of glucose, *Anal. Biochem.*, **519** (2017), pp. 19–26.
- [51] A. K. Geim, K. S. Novoselov, The rise of graphene, *Nat. Mater.* **6** (2007), pp. 183–191.
- [52] D. A. C. Brownson, C. E. Banks, Graphene electrochemistry: An overview of potential applications, *The Analyst*, **135** (2010), pp. 2768–2778.
- [53] S. Rathinavel, K. Priyadarshini, D. Panda, A review on carbon nanotube: An overview of synthesis, properties, functionalization, characterization, and the application, *Mat. Sci. Eng. B*, **268** (2012), pp. 115095 [doi.org/10.1016/j.mseb.2021.115095](https://doi.org/10.1016/j.mseb.2021.115095)



- [54] S. Mallakpour, S. Soltanian, Surface functionalization of carbon nanotubes: fabrication and applications, *RSC Adv.*, **6** (2016), pp. 109916–109935.
- [55] R. Dubey, D. Dutta, A. Sarkar, P. Chatopadhyay, Functionalized carbon nanotubes: synthesis, properties and applications in water purification, drug delivery, and material and biomedical sciences, *Nanoscale Adv.*, **3** (2021), pp. 5722–5744.
- [56] V. Georgakilas, M. Otyepka, A. B. Bourlinos, V. Chandra, N. Kim, K. C. Kemp, P. Hobza, R. Zboril, K. S. Kim, Functionalization of graphene: Covalent and non-covalent approaches, derivatives and applications, *Chem. Rev.*, **112** (2012), pp. 6156–6214.
- [57] M. M. Barsan, M. E. Ghica, C. M. A. Brett, Electrochemical sensors and biosensors based on redox polymer/carbon nanotube modified electrodes: A review, *Anal. Chim. Acta*, **881** (2015), pp. 1–23.
- [58] R. Kour, S. Arya, S.-J. Young, V. Gupta, P. Bandhoria, A. Khosla, Recent advances in carbon nanomaterials as electrochemical biosensors, *J. Electrochem. Soc.*, **167** (2020), 037555.
- [59] J. Wang, Carbon-nanotube based electrochemical biosensors: A review, *Electroanalysis*, **17** (2005), pp. 7–14.
- [60] A. Casanova, J. Iniesta, A. Gomes-Berenguer, Recent progress in development of porous carbon-based electrodes for sensing applications, *The Analyst*, **147** (2022), pp. 767–783.
- [61] S. A. David, R. Rajkumar, P. Karpagavinayagam, J. Fernando, C. Vedhi, Sustainable carbon nanomaterial-based sensors: Future vision for the next 20 years, *Carbon Nanomaterials-Based Sensors*, **1** (2022), pp. 429–443, 10.1016/B978-0-323-91174-0.00011-1.
- [62] A. T. Lawal, H. S. Bolarinwa, M. D. Adeoye, I. O. Abdulsalami, L. O. Animasahun, K. A. Alabi, Progress in carbon nanotube-based electrochemical biosensors-A review, *FUJNAS*, **8** (2019), pp. 38–74.
- [63] P. Das, M. Das, S. R. Chinnadayala, I. M. Singha, P. Goswami, Recent advances on developing 3rd generation enzyme electrode for biosensor applications, *Biosens. Bioelectron.* **79** (2016), pp. 386–397.
- [64] S. Gupta, C. N. Murthy, C. Ratna Prabha, Recent advances in carbon nanotube based electrochemical biosensors, *Int. J. Biol. Macromol.* **108** (2018), pp. 687–703.
- [65] G. S. Wilson, R. Gifford, Biosensors for real-time in vivo measurements, *Biosens. Bioelectron.*, **20** (2005), pp. 2388–2403.
- [66] S. Berger, M. Berger, C. Bantz, M. Maskos, E. Wagner, performance of nanoparticles for biomedical applications: The in vivo/in vitro discrepancy, *Biophysics Rev.*, **3** (2022), 011303 DOI:doi.org/10.1063/5.0073494.
- [67] D. C. Ferrier, K. C. Honeychurch, Carbon nanotube (CNT)-based biosensors, *Biosensors*, **11** (2021), 486 doi.org/10.3390/bios11120486
- [68] D. Bhatnagar, S. K. Tuteja, R. Rastogi, L. M. Bharadwaj, Label-Free Detection of Hemoglobin Using MWNT-Embedded Screen-Printed Electrode, *BioNanoScience*, **3** (2013), pp. 223–231.
- [69] A. P. Periasamy, Y. J. Chang, S. M. Chen, Amperometric glucose sensor based on glucose oxidase immobilized on gelatin-multiwalled carbon nanotube modified glassy carbon electrode, *Bioelectrochem.*, **80** (2011), pp. 114–120.
- [70] Y. C. Tsai, J. D. Huang, C. C. Chiu, Amperometric ethanol biosensor based on poly(vinyl alcohol)-multiwalled carbon nanotube-alcohol dehydrogenase biocomposite, *Biosens. Bioelectron.*, **22** (2007), pp. 3051–3056.
- [71] J. N. Ashby, R. P. Ramasamy, Molecularly Tethered Cholesterol Oxidase on Multiwall Carbon Nanotubes for Indirect Detection of Cholesterol, *ECS Trans.*, **69** (2015), pp. 1–9.
- [72] B. Dalkiran, P. E. Erden, E. Kilic, Amperometric biosensors based on carboxylated multiwalled carbon nanotubes-metal oxide nanoparticles-7, 8, 8-tetracyanoquinodimethane composite for the determination of xanthine, *Talanta*, **167** (2017), pp. 286–295.
- [73] A. K. Deb, S. C. Das, A. Saha, M. B. Wayu, M. H. Marksberry, R. J. Baltz, C. C. Chusuei, Ascorbic acid, acetaminophen, and hydrogen peroxide detection using a dendrimer-encapsulated Pt nanoparticle carbon nanotube composite, *J. App. Electrochem.*, **46** (2016), pp. 289–298.
- [74] S. Draminska, R. Bilewicz, Bienzymatic mediatorless sensing of total hydrogen peroxide with catalase and multi-copper enzyme co-adsorbed at carbon nanotube-modified electrodes. *Sensors and Actuators, B: Chemical*, **248** (2017), pp. 493–499.
- [75] B. Ertek, Y. Dilgin, Photoamperometric flow injection analysis of glucose based on dehydrogenase modified quantum dots-carbon nanotube nanocomposite electrode, *Bioelectrochem.*, **112** (2016) pp. 138–144.
- [76] J. Huan, Y. Li, J. Feng, M. Li, P. Wang, Z. Chen, Y. Dong, A novel sandwich-type immunosensor for detection of carcino-embryonic antigen using silver hybrid multiwalled carbon nanotubes/manganese dioxide, *J. Electroanal. Chem.*, **786** (2017), pp. 112–119.
- [77] A. Quang Dao, D. M. Nguyen, T. T. T. Toan, The modified glassy carbon electrode by MWCNTs-PLL to detect both paracetamol and ibuprofen in human biological fluid, *J. Electrochem. Soc.*, **169** (2022), 057525 10.1149/1945-7111/ac6f89
- [78] G. X. Ma, T. H. Lu, Y. Y. Xia, Direct electrochemistry and bioelectrocatalysis of hemoglobin immo-

- bilized on carbon black, *Bioelectrochem.*, **71**(2007), pp. 180–185.
- [79] E. V. Suprun, F. Arduini, D. Moscone, G. Palleschi, V. V. Shumyantseva, A. I. Archakov, Direct electrochemistry of hem proteins on electrodes modified with didodecylmethyl ammonium bromide and carbon black, *Electroanalysis*, **24** (2012), pp. 1923–1931.
- [80] C. Dai, Y. Ding, M. Li, J. Fei, Direct electrochemistry of cytochrome P450 in a biocompatible film composed of epoxy polymer and acetylene black, *Microchim. Acta*, **176** (2012), pp. 397–404.
- [81] R. K. Satvekar, Electrochemical nanobiosensors perspectives for COVID 19 pandemic, *J. Electrochem. Sci. Eng.*, **12** (2022), pp. 25–35.
- [82] J. Chen, S. Chen, X. Zhao, L. V. Kuznetsova, S. S. Wong, I. Ojima, Functionalized single-walled carbon nanotubes as rationally designed vehicles for tumor-targeted drug delivery, *J. Am. Chem. Soc.*, **130** (2008), pp. 16778–16785.
- [83] J. Shi, L. Wang, J. Gao, . Liu, J. Zhang, R. Ma, R. Liu, Z. Zhang, A fullerene-based multi-functional nanoplatform for cancer theranostic applications, *Biomaterials*, **35** (2014) pp. 5771–5784.
- [84] R. D. Bolskar, Gadofullerene MRI contrast agents, *Nanomedicine*, **3** (2008), 201–213.
- [85] P. V. Jena, T. V. Galassi, D. Roxbury, D. A. Heller, Progress towards applications of nanotube photoluminescence, *ECS J. Solid State Sci. Technol.*, **6** (2017), pp. M3075-M3077.
- DOI: 10.1149/2.0121706jss
- [86] A. Dellinger, Z. Zhou, J. Connor, A. B. Madhankumar, S. Pamujula, Application of fullerenes in nanomedicine; an update, *Nanomedicine*, **8** (2013), pp. 1191–1208.
- [87] R. Gulaboski, V. Mirceski, Application of voltammetry in biomedicine-Recent achievements in enzymatic voltammetry, *Maced. J. Chem. Chem. Eng.*, **39** (2020), pp. 153–166.
- [88] R. Gulaboski, Electrochemistry in 21<sup>st</sup> century-Future trend and perspectives, *J. Solid State Electrochem.*, **24** (2020). doi: 10.1007/s10008-020-04550-0
- [89] F. Kuralay, *Nanomaterials-based enzyme biosensors for electrochemical applications: Recent trends and future prospects*; In: *New developments in nanosensors for pharmaceutical analysis*, Academic Press, 2019, pp. 381–408.
- [90] A. A. Atiyah, A. J. Haider, R. M. Dhahi, Cytotoxicity properties of functionalized carbon nanotubes on pathogenic bacteria, *IET Nanobiotechnol.*, **13** (2019), pp. 597–601.
- [91] K. E. Kitko, Q. Zhang, Graphene-based nanomaterials: From production to integration with modern tools in neuroscience, *Front. Syst. Neurosci.*, **13** (2019).DOI: doi.org/10.3389/fnsys.2019.00026
- [92] G. Tigari, J. G. Manjunatha, H. Nagarajappa, N. S. Prinith, Research developments in carbon materials based sensors for determination of hormones, *J. Electrochem. Sci. Eng.*, **12** (2022) pp. 3–23.